

## Creatine Kinase-MB Assay Kit (CK-MB)

Method: DGKC

Cat .No.	Size	Instrument
GB210X	R1: 2×40 ml R2: 1×20 ml	For Hitachi 717 & ShimadzuCL7200/8000
GS211X	R1: 4×20 ml R2: 1×20 ml	For Hitachi917 & OlympusAU640/400/600
GH211X	R1: 2×40 ml R2: 1×20 ml	For Hitachi902
GX211X	R1: 1×80 ml R2: 1×20 ml	For SYNCHRON CX4-5-7- 9/LX20/DXC600-800
GT211X	R1: 2×40 ml R2: 1×20 ml	For TOSHIBA

### INTENDED USE


For the *in vitro* quantitative determination of creatine kinase -MB (CK-MB) in human serum .

### CLINICAL SIGNIFICANCE

CK-MB is present in low concentration in normal human serum but is increased as a result of heart injury, and rarely, skeletal muscle damage. CK-MB is widely used as an indicator of acute myocardial infarction as the detection of elevated activities is considered highly specific for this condition.

### ASSAY PRINCIPLE

Creatine Kinase is a dimer. Its monomeric subunits are designated M and B. The subunits combine to form three isoenzymes namely CKBB, CK-MB and CK-MM. CK-MM and CK-MB are found primarily in skeletal and heart muscle, respectively, while CK-BB is found mainly in the brain and smooth muscle tissue. In serum, the CK-BB activity can be ignored. M Subunits of CK-MM and CK-MB are inactivated by reaction with anti-M antibody (immunoinhibition). The remaining B-subunit is measured enzymatically.

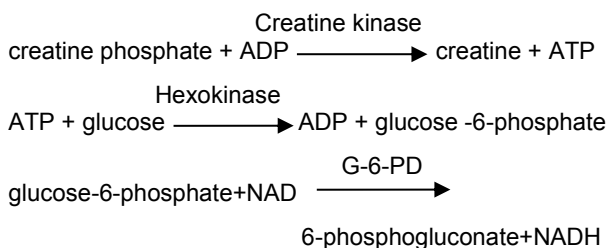

Through a series of coupled enzymatic reactions, NADH is produced at a rate directly proportional to the CK B subunit activity. Multiply the activity by 2, and this result is just the activity of CK-MB.

### SAMPLE COLLECTION AND PREPARATION

Serum samples. Samples are stable for 4 hours at temperature, for 8 hours at 2-8°C, for 2 days at -20°C.

### REAGENT COMPOSITION

Contents	Concentration
Imidazole buffer pH6.7	100 mmol/L
Creatine phosphate	30 mmol/L

Glucose	20 mmol/L
N-Acetylcysteine (NAC)	20 mmol/L
MgAC	10 mmol/L
EDTA	2 mmol/L
ADP	2 mmol/L
AMP	5 mmol/L
Diadenosine pentaphosphate	10 μmol/L
G6PDH	≥1.5 KU/L
HK	≥2.5 KU/L
NADP	2 mmol/L
Anti-M subunit polyclonal antibody	≥ 2KU/L

### STABILITY AND PREPARATION OF REAGENTS

All reagents are ready to use.

Stable up to the expiry date when stored at 2-8°C.


The reagent after opening is stable for 28 days on-board the analyser .

### ASSAY PROCEDURE

**Test Procedure for Analyzers (HITACHI 917)**

Assay Mode: Rate

Wave Length (main/sub): 340 nm/ 410 nm

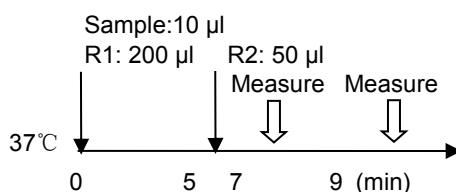

- Mix 10 μl sample with 200 μl R1 and incubate at 37°C for 5 minutes.
- Add 50 μl R2 into cuvette, mix and incubate at 37°C for 2 minutes.
- Read initial absorbance and start timer simultaneously, read again after 1, 2 and 3 minutes.
- Calculate absorbance change per minute (ΔA/min)

### CALCULATION

Using K factor

$$\begin{aligned}
 \text{CK-MB (U/L)} &= \frac{\Delta A/\text{min} \times V_t}{\epsilon \times V_s \times L} \times 1000 \times 2 \\
 &= \Delta A/\text{min} \times K \\
 K &= 8255 \quad (37^\circ\text{C})
 \end{aligned}$$

### QUALITY CONTROL

For quality control, use Control as daily quality control sera and can be purchased separately. Values should fall within a specific range. If these values fall outside the range and repetition excludes error, the following steps should be taken:

- Check instrument settings and light source.
- Check reaction temperature.
- Check expiration date of kit and contents.
- Check the quality of the water used for reagents reconstitution.

### NORMAL VALUE

CK-MB: < 25 U/L

It is recommended that each laboratory establish its own reference range to reflect the age, sex, diet and geographical location of the population.

## SPECIFIC PERFORMANCE CHARACTERISTICS

### LINEARITY

The method is linear up to 600 U/L. If the sample above this concentration should be diluted 1+1 with 0.9% NaCl and repeat assay. Multiply the result by 2.

### PRECISION

The CV of the test should be less than 10%

Intra assay precision	
N=15	Level 1
Mean(U/L)	115.43
SD(U/L)	0.385
CV	0.33%
Inter assay precision	
N=5	Level 1
Mean (U/L)	115.61
SD(U/L)	0.266
CV	0.23%

### SENSITIVITY

The minimum detectable level that can be distinguished from zero has been determined as 5 U/L.

### INTERFERENCE

The following analytes were tested up to the levels indicated and found not to interfere:

Intralipid:	2000 mg/dl
Hemoglobin:	500 mg/dl
Direct bilirubin:	40 mg/dl
Ascorbic Acid:	50 mg/dl

### CORRELATION

This method (Y) was compared with another commercially available method (X) and the following linear regression equation obtained:

$Y=1.0048X+0.2362$ , and a correlation coefficient of 0.9989; 50 patient samples were analyzed.

### SAFETY PRECAUTIONS AND WARNINGS

- For in vitro diagnostic use only. Do not pipette by mouth. Exercise the normal precautions required for handling laboratory reagents.
- The reagents contains Sodium Azide. Avoid ingestion or contact with skin or mucous membranes. In case of skin contact, flush affected area with copious amounts of water. In case of contact with eyes or if ingested, seek immediate medical attention.
- Sodium Azide reacts with lead and copper plumbing, to form potentially explosive azides. When disposing of such reagents flush with large volumes of water to prevent azide build up. Exposed metal surfaces should be cleaned with 10% sodium hydroxide.
- All specimens used in this test should be considered potentially infectious. Universal Precautions, as they apply at your facility, should be used for handling and disposing of materials during and after testing.

## REFERENCES

- Tietz, N. W, Textbook of Clinical Chemistry, W.B. Saunders Co, Philadelphia, 1986, p. 678-6863.
- Szasz, G., et al. Clin. Chem 1976; 22: 650.
- Recommendations of the German Society for Clinical Chemistry. Standardization of methods for the estimation of enzyme activities in biological fluids: Standard method for the determination of creatine kinase activity. J Clin Chem Clin Biochem 1977; 15:255-60.

## INDEX OF SYMBOLS



Manufacture



Catalogue Number



Lot number



Date of manufacture



Use by (Expiration date)




For In-Vitro Diagnostic use only



Stored at 2-8°C



Attention: See instruction for use



Authorized Representative in the European Company

Manufacture: Beijing Strong Biotechnology, Inc.

Address : No. 15, Yanqi North Second Street, Yanqi Economic Development Area, Huairou District, Beijing 101400, P. R. China

Tel: +86 10 61667168

EC REP :Lotus NL B.V.

Address : Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands.

E-mail: peter@lotusnl.com

Tel: +31645171879(English), +31626669008 (Dutch)